



Applicant(s): Nigel P. Gore

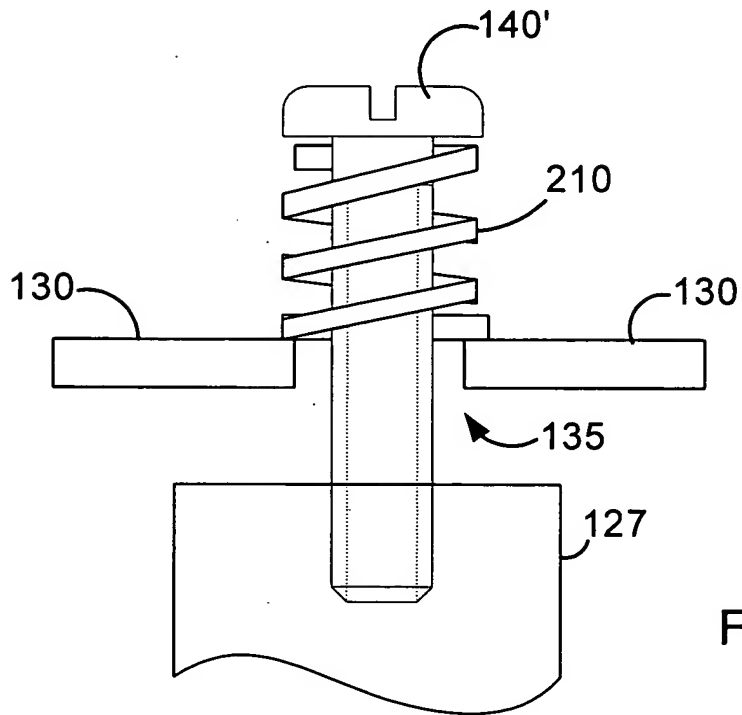
DECREASING LOAD ON DEVICES FOR MASS  
SPECTROMETERS

FIG. 2A

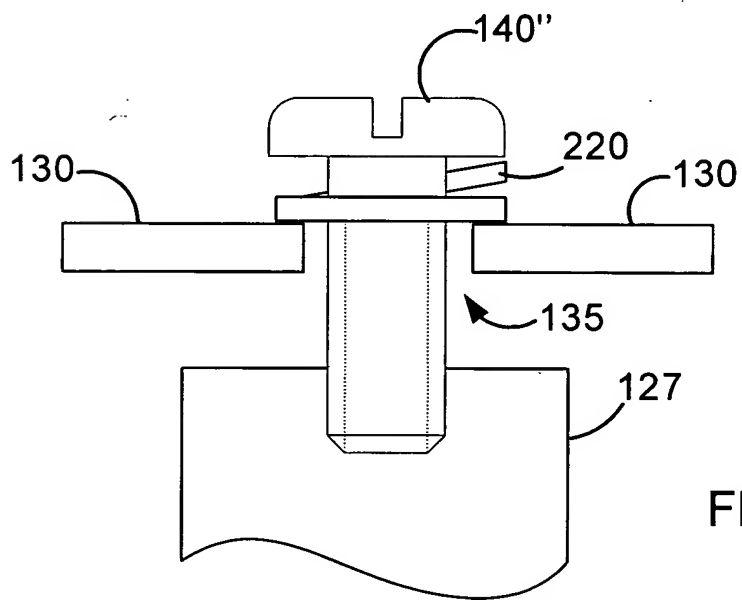
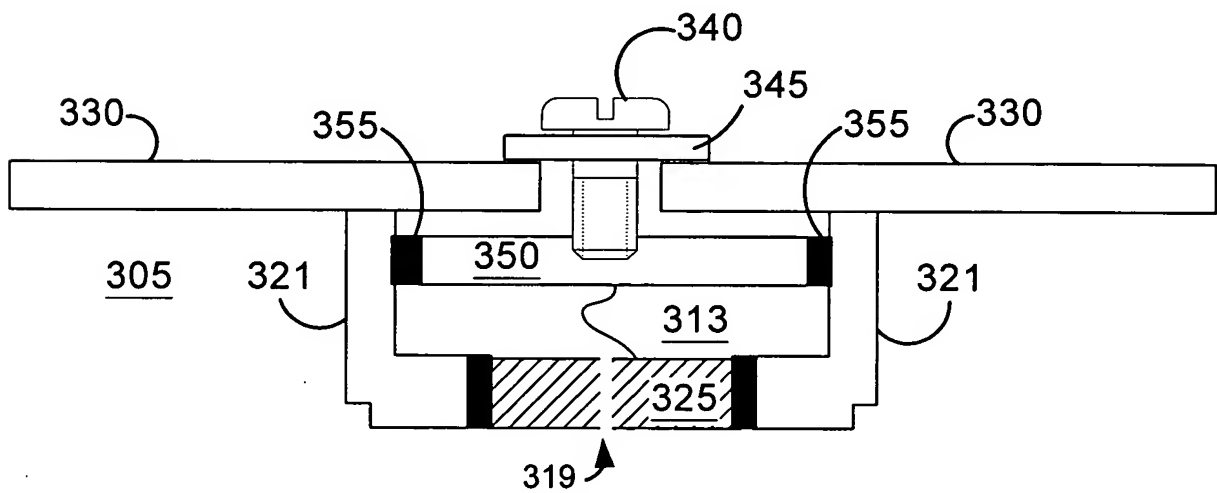
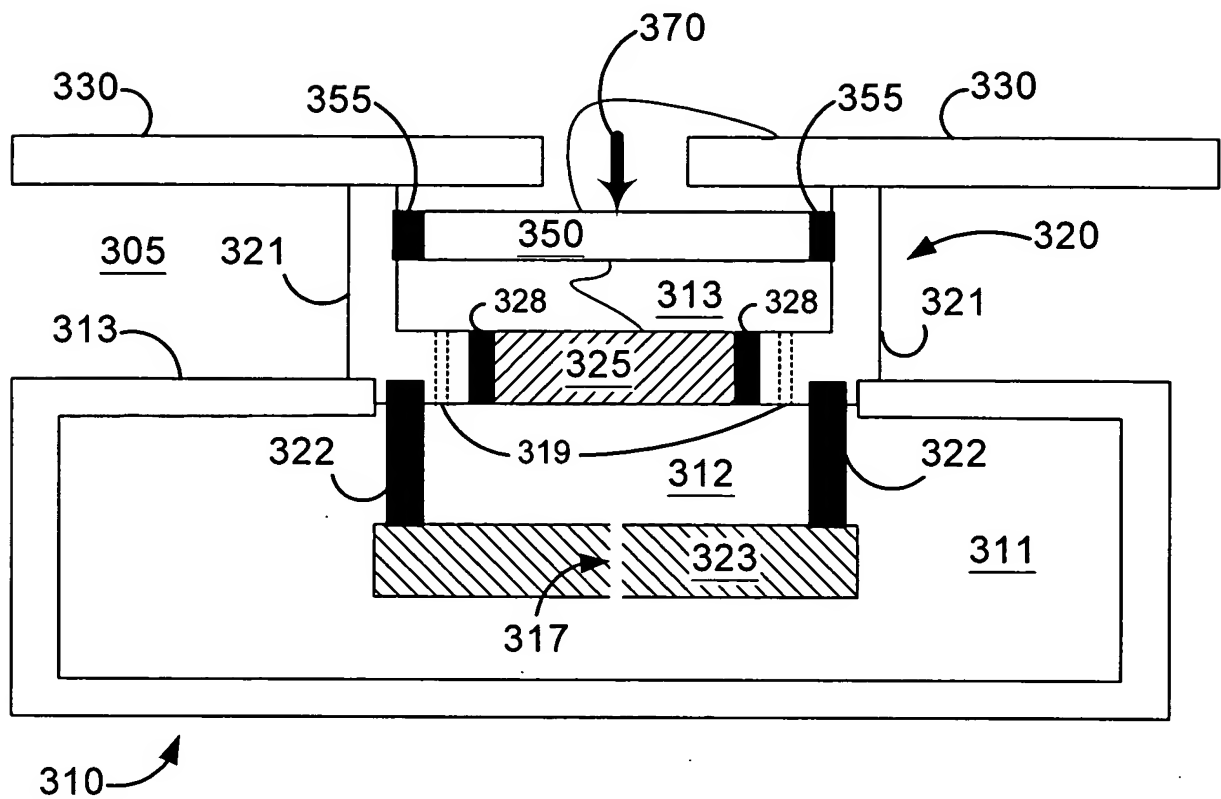


FIG. 2B



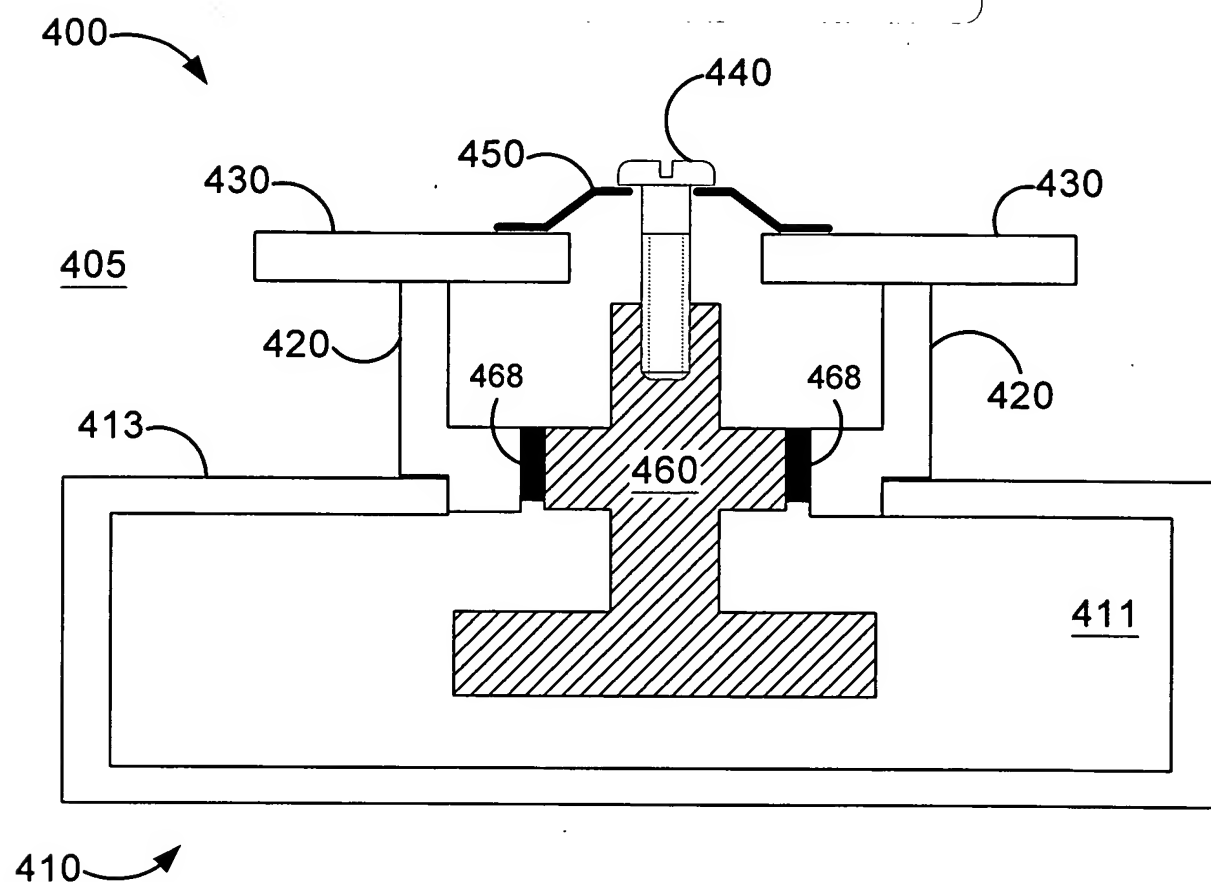


FIG. 4

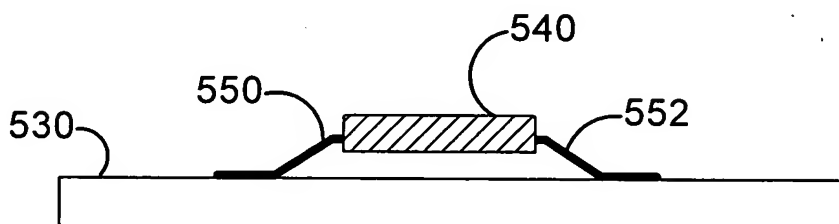


FIG. 5